EXHIBIT 17

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

Claim	Accused Product
[1.pre] An electronic device for long-term adhesion to a user, the device comprising:	To the extent the preamble is limiting, the Bardy CAM Patch product comprises an electronic device for long-term adhesion to a user, the device comprising. The Bardy CAM Patch product comprises an electronic device that is adhered to a user. 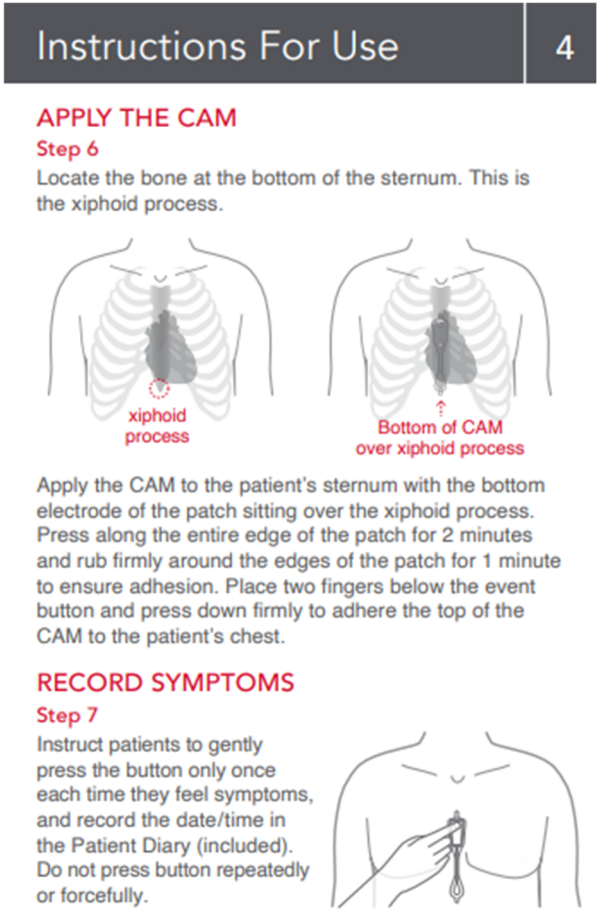 (https://www.bardydx.com/wp-content/uploads/2023/06/DWG000781B-CAM-Instructions-for-

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

	Use.pdf) 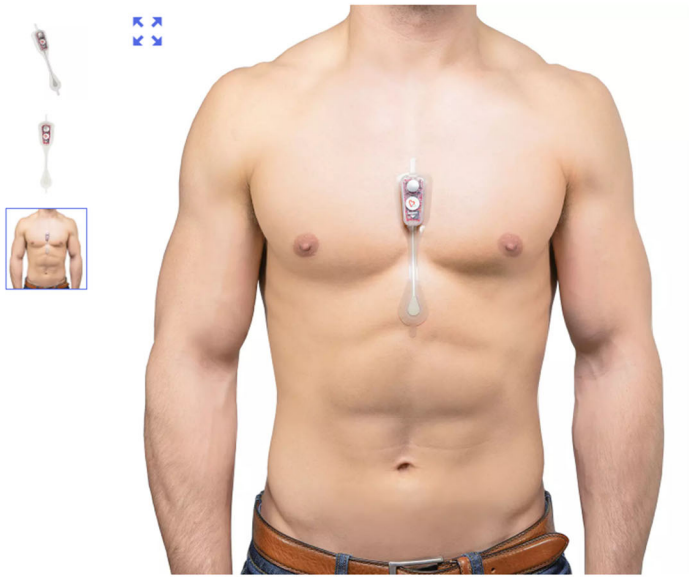 (https://www.hillrom.com/en/products/cam-patch/; *see also* https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM-Brochure.pdf) The Bardy CAM Patch comprises long-term adhesion, for example, for the service life of the Patch of "[u]p to 2, 7, or 14 days."

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

	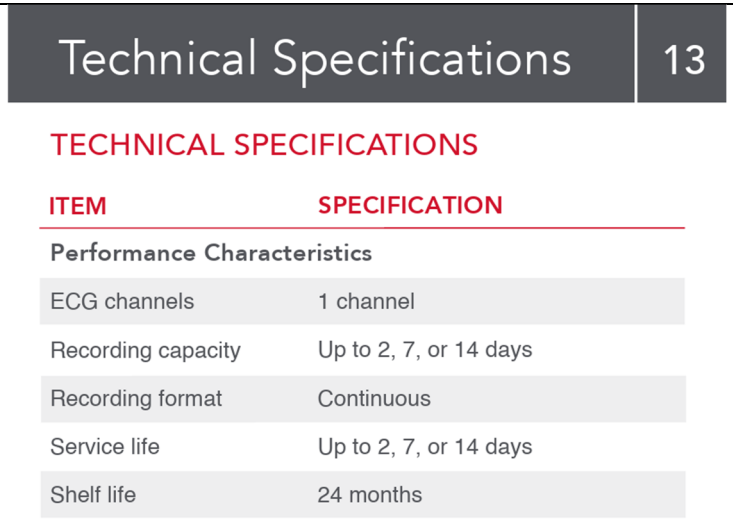 (https://www.bardydx.com/wp-content/uploads/2023/06/DWG000781B-CAM-Instructions-for-Use.pdf)
[1.a] a housing comprising a physiological data collection circuit,	The Bardy CAM Patch product comprises a housing comprising a physiological data collection circuit. For example, the Bardy CAM Patch product includes a physiological data collection circuit. A circuit in the Bardy CAM Patch collects physiological data, such as cardiac P-wave signals.

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

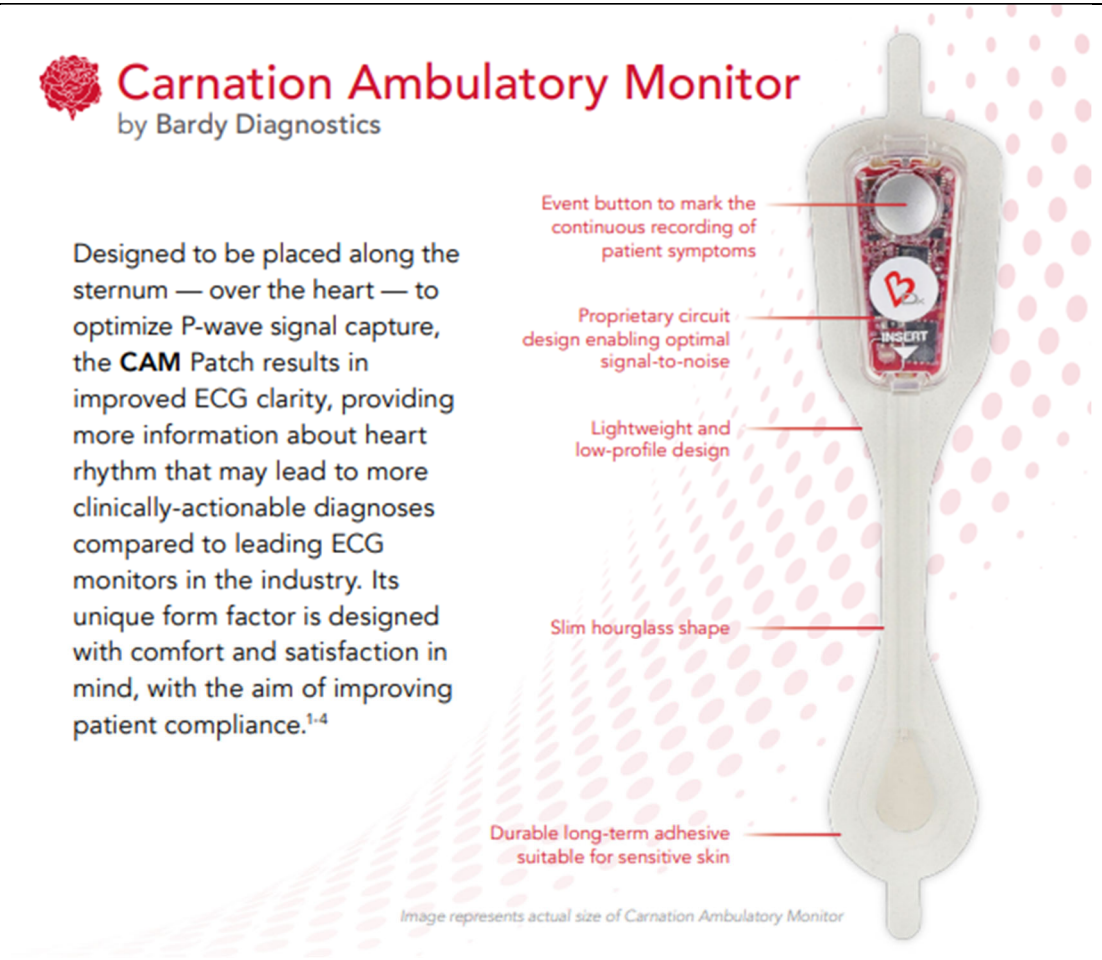

(https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM-Brochure.pdf)

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

Convenience for the Practice

Customizable Workflow to Fit the Needs of Your Practice[1]

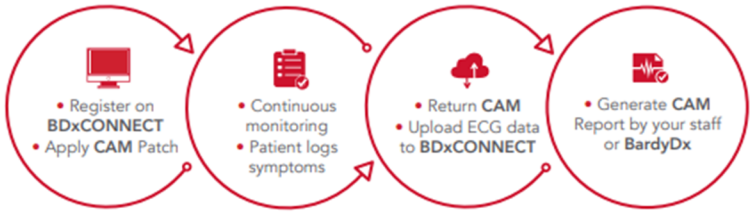

Increased Efficiency and Streamlined Clinical Workflows Using our Easy-to-Use Patient Management Portal[4]

- Fast Access to Reports by Direct Upload of Patient Data
- Flexibility to do own Analysis or Utilize our Certified Techs
- 2-Day Report Turnaround
- Secure Cloud-Based Network

Clarity for the Physician[2]

ECG Clarity That Improves Clinical Decision Making[2-4]

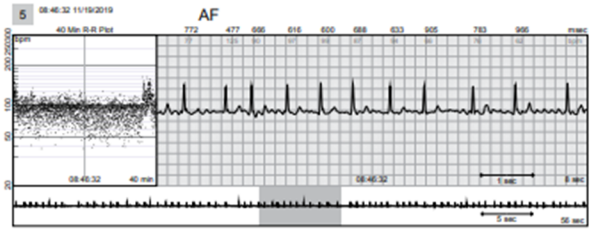

- High Diagnostic Yield for Informed Diagnoses[1-3]
- 14 Days Extended Duration Monitoring
- Proprietary Report Format Delivers Clarity and Context[1]

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

	(https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM-Brochure.pdf) The Bardy CAM Patch product includes a housing that comprises a physiologic data collection circuit.  (https://youtu.be/RPcdb-volpc?si=meNXw98UDtIgwqp1&t=126)
[1.b] the housing positioned over a flexible layer extending from beneath the housing, the flexible layer comprising an electrode positioned on the bottom of the flexible layer at a position distal from the housing,	The Bardy CAM Patch product comprises the housing positioned over a flexible layer extending from beneath the housing, the flexible layer comprising an electrode positioned on the bottom of the flexible layer at a position distal from the housing, For example, the Bardy CAM Patch product includes a housing positioned over a flexible layer extending from beneath the housing.

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

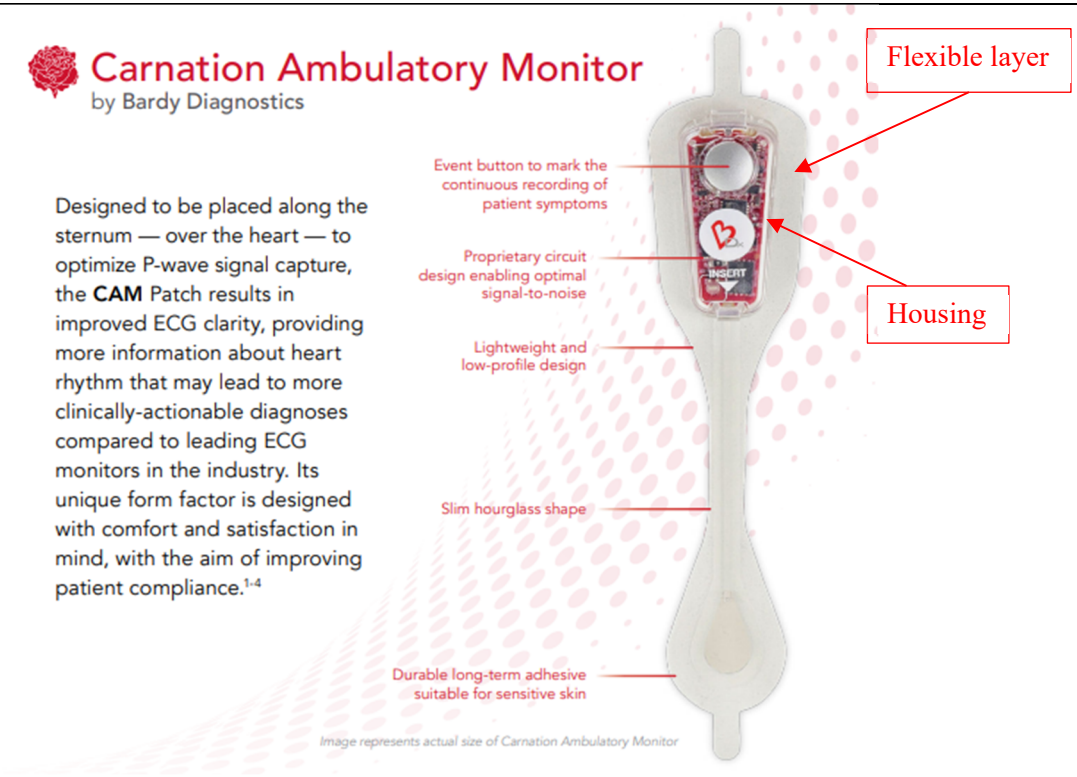

(https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM-Brochure.pdf)

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

	 (https://youtu.be/RPcdb-volpc?si=meNXw98UDtIgwqp1&t=126). For example, the Bardy CAM Patch product includes a flexible layer comprising an electrode positioned on the bottom of the flexible layer at a position distal from the housing.

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

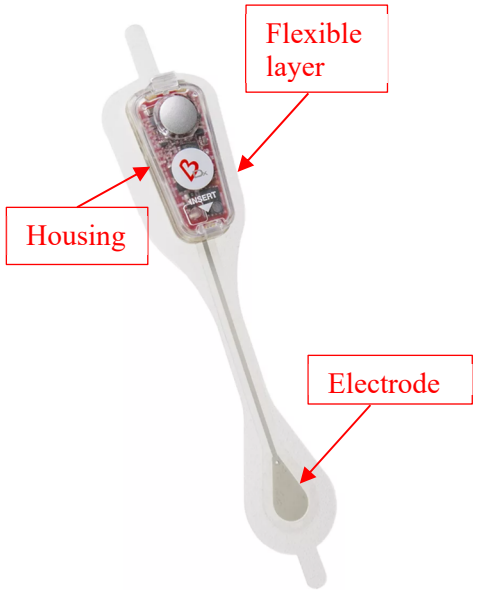

Baxter

CAM Patch

The CAM Patch is a long-term ambulatory ECG monitor that has been clinically proven to identify arrhythmias. It is engineered to optimize p-wave signal capture, which enables differentiation between different types of atrial, as well as ventricular, arrhythmias[1,2]. The CAM's simple design allows for ease of application and its clinical portal helps streamline clinician workflow.

Learn more about the **CAM** Patch solution.

Request More Information ›

(https://www.hillrom.com/en/products/cam-patch/)

BardyDx® Carnation Ambulatory Monitor (CAM®) Specifications

ELECTRODE CHARACTERISTICS

ITEM	SPECIFICATION
Number of electrodes	2
Type	Electrode incorporating electrode gel and internal lead wire
Supplied as	Disposable, non-sterile
Lead wire length	11.6 cm (no patient contact)
Materials	Electrode gel: Medical grade conductive synthetic Adhesive: Medical grade skin adhesive

(https://www.bardydx.com/wp-content/uploads/2025/01/DN000697B-BDx_CAM_SpecSheet.pdf)

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

[1.c] wherein the flexible layer comprises a polymer upper layer overlying an electrical connection, the electrical connection extending linearly from the physiologic data collection circuit to the electrode when viewed from above the electronic device, the polymer upper layer adhered to a polymer lower layer underlying the electrical connection;	The Bardy CAM Patch product comprises wherein the flexible layer comprises a polymer upper layer overlying an electrical connection, the electrical connection extending linearly from the physiologic data collection circuit to the electrode when viewed from above the electronic device, the polymer upper layer adhered to a polymer lower layer underlying the electrical connection. For example, the Bardy CAM Patch includes a flexible layer comprising a polymer upper layer overlying an electrical connection. 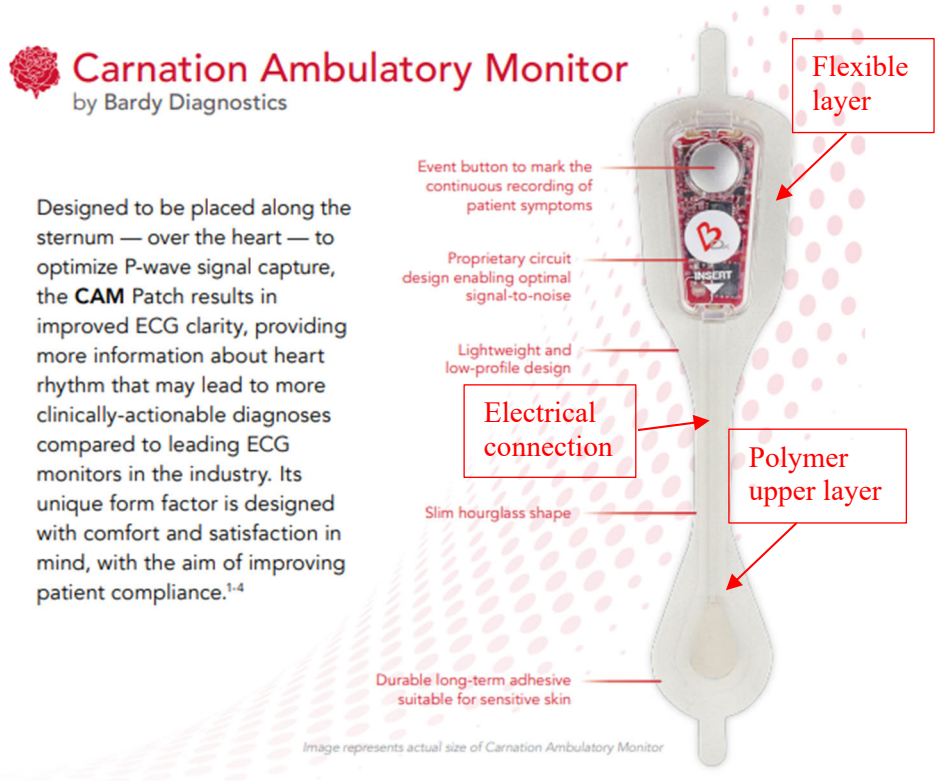 (https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM-Brochure.pdf)

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

	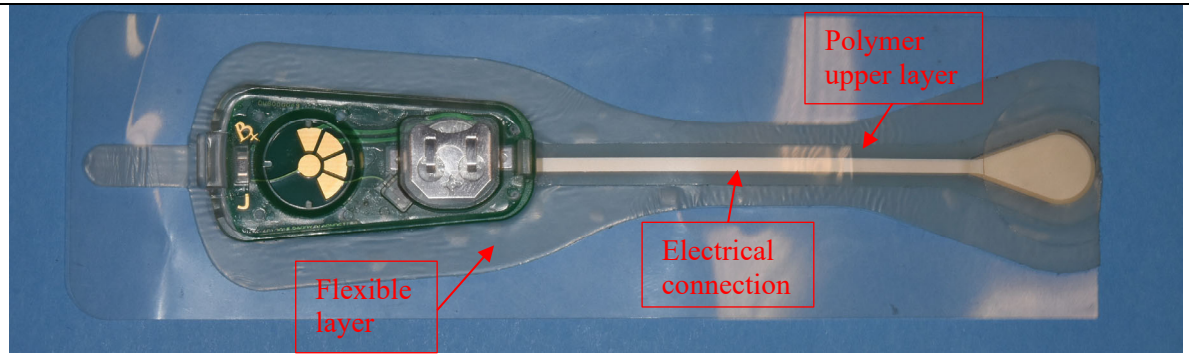 For example, the Bardy CAM Patch includes the electrical connection extending linearly from the physiologic data collection circuit to the electrode when viewed from above the electronic device.

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

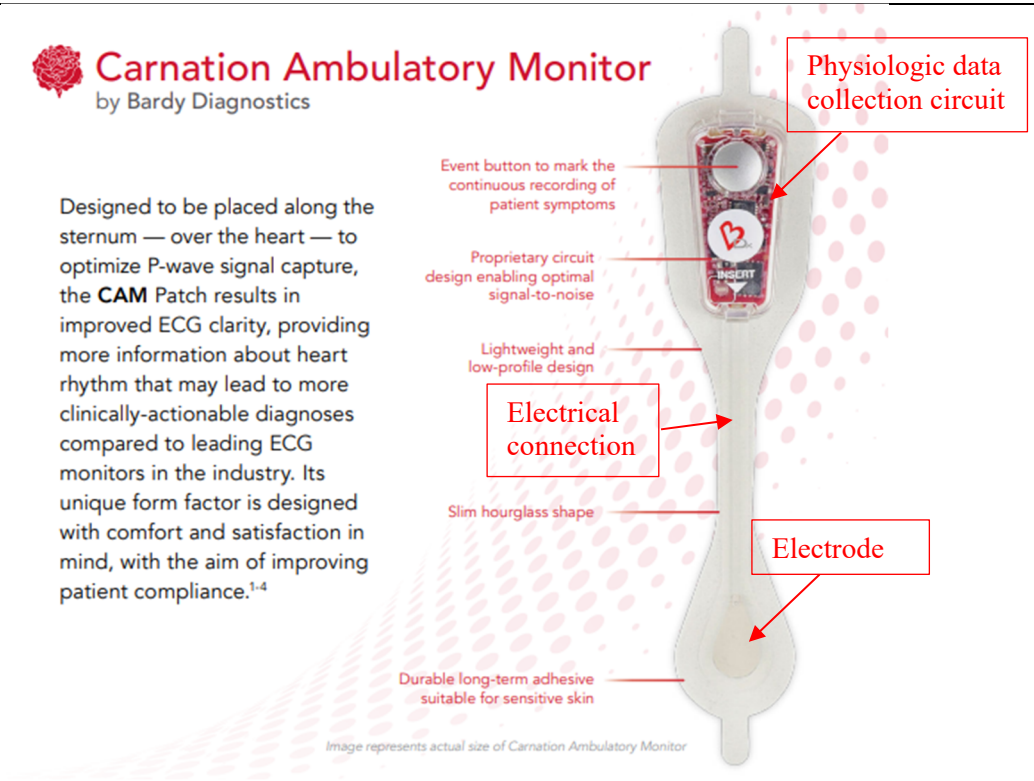

(https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM-Brochure.pdf)

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

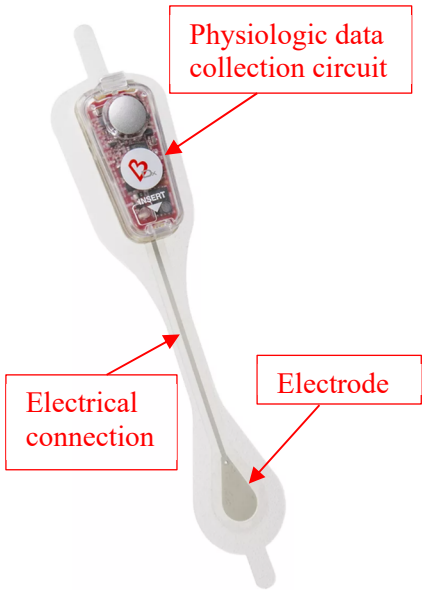

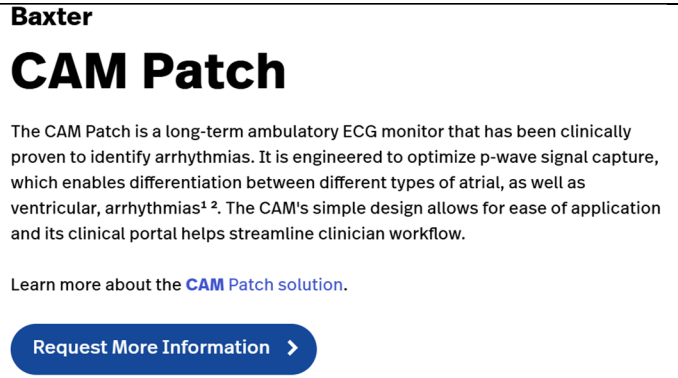

(https://www.hillrom.com/en/products/cam-patch/)

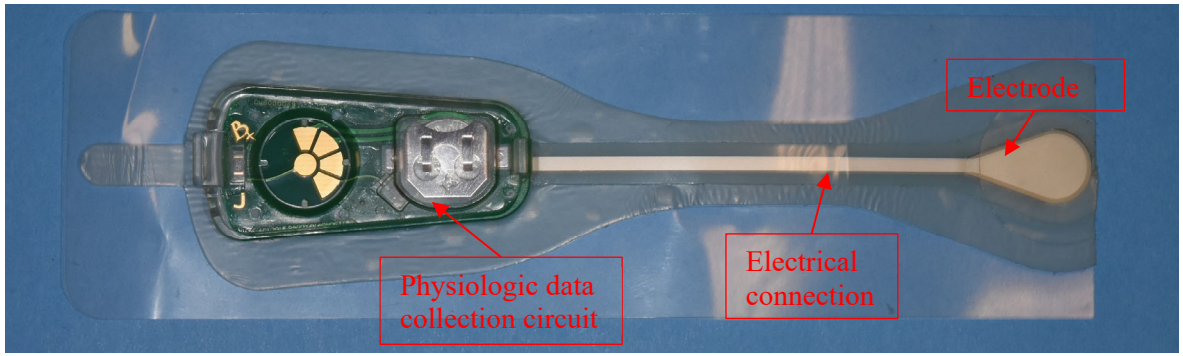

For example, the Bardy CAM Patch includes a polymer upper layer adhered to a polymer lower layer underlying the electrical connection.

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

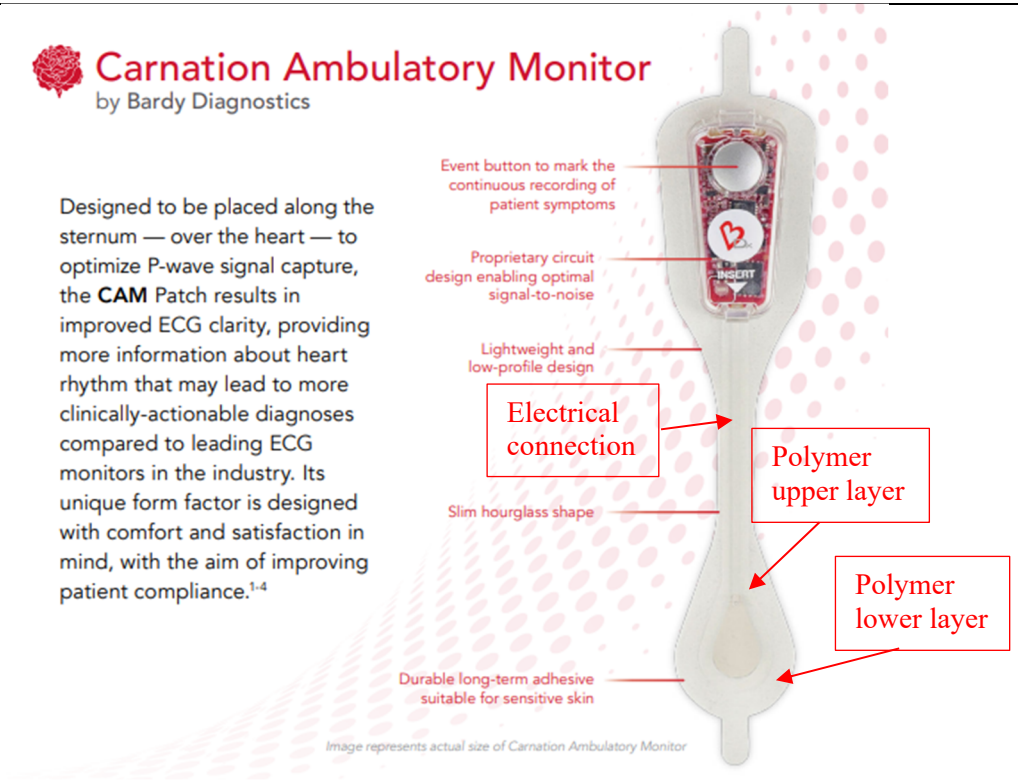

(https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM-Brochure.pdf)

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

	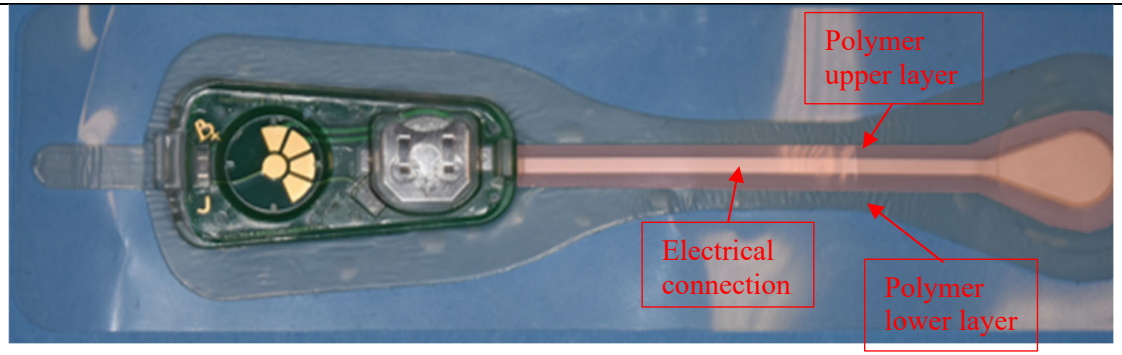
[1.d] a connecting adhesive layer positioned under the polymer upper layer, the connecting adhesive layer adhering the polymer upper layer to the polymer lower layer; and	The Bardy CAM Patch product comprises a connecting adhesive layer positioned under the polymer upper layer, the connecting adhesive layer adhering the polymer upper layer to the polymer lower layer; and. For example, the Bardy CAM Patch product comprises a connecting adhesive layer. The Bardy CAM Patch product includes a polymer upper layer that is adhered to a polymer lower layer via a connecting adhesive layer located under the polymer upper layer. 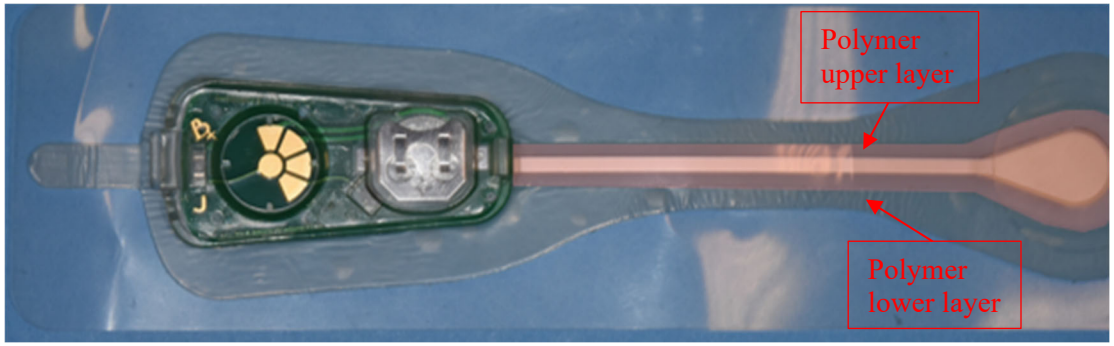
[1.e] a lower adhesive layer positioned on the flexible layer and configured to adhere the electronic device to a user.	The Bardy CAM product comprises a lower adhesive layer positioned on the flexible layer and configured to adhere the electronic device to a user. For example, the Bardy CAM Patch product comprises a lower adhesive layer positioned on the flexible

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

	layer and configured to adhere the electronic device to a user. Step 5 Gently peel the liner from the CAM by grasping the tab at the top of the device and peeling downward, carefully avoiding contact with the adhesive.  ⚠ CAUTION: Touching the adhesive can reduce adhesive performance. Hold onto tabs at the end of the CAM. (https://www.bardydx.com/wp-content/uploads/2023/06/DWG000781B-CAM-Instructions-for-Use.pdf)

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

	Instructions For Use 4 APPLY THE CAM Step 6 Locate the bone at the bottom of the sternum. This is the xiphoid process. 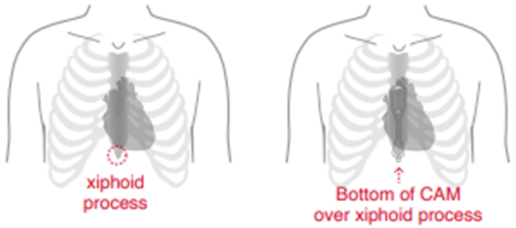 Apply the CAM to the patient's sternum with the bottom electrode of the patch sitting over the xiphoid process. Press along the entire edge of the patch for 2 minutes and rub firmly around the edges of the patch for 1 minute to ensure adhesion. Place two fingers below the event button and press down firmly to adhere the top of the CAM to the patient's chest. (https://www.bardydx.com/wp-content/uploads/2023/06/DWG000781B-CAM-Instructions-for-Use.pdf)

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

Baxter

CAM Patch

The CAM Patch is a long-term ambulatory ECG monitor that has been clinically proven to identify arrhythmias. It is engineered to optimize p-wave signal capture, which enables differentiation between different types of atrial, as well as ventricular, arrhythmias[1] [2]. The CAM's simple design allows for ease of application and its clinical portal helps streamline clinician workflow.

Learn more about the CAM Patch solution.

Request More Information >

(https://www.hillrom.com/en/products/cam-patch/; *see also* https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM-Brochure.pdf)

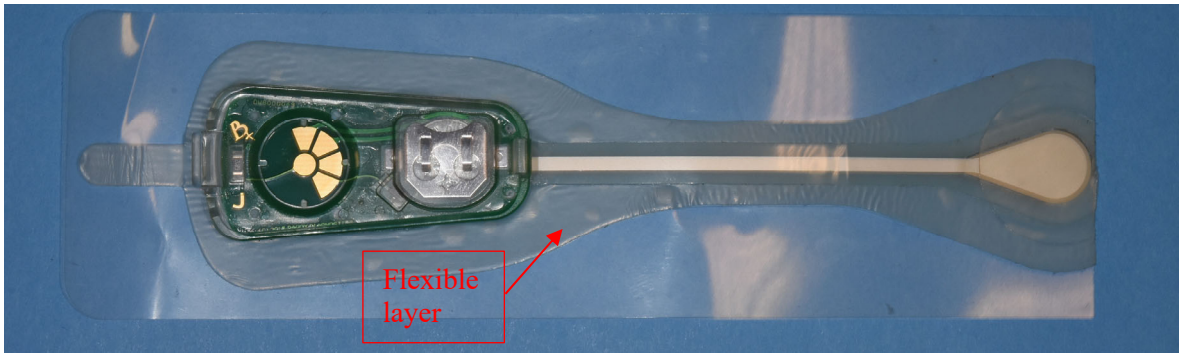

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

	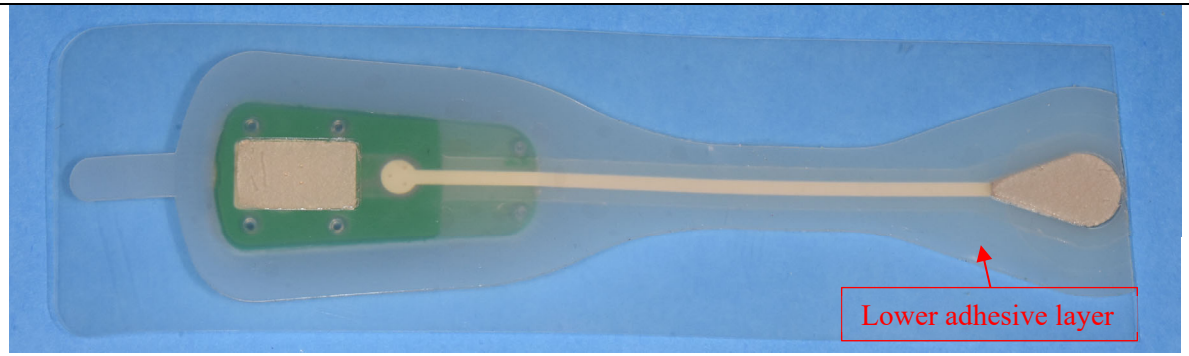
[4] The electronic device of claim 1, wherein the housing is configured to remain connected to the flexible layer when the housing is tilted at an angle relative the lower adhesive layer in response to movement of the user.	The Bardy CAM product comprises the electronic device of claim 1, wherein the housing is configured to remain connected to the flexible layer when the housing is tilted at an angle relative the lower adhesive layer in response to movement of the user. For example, the Bardy CAM Patch product comprises the electronic device of claim 1, as explained above. For example, the Bardy CAM Patch product comprises a housing configured to remain connected to the flexible layer when the housing is tilted at an angle relative the lower adhesive layer in response to movement of the user.

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

	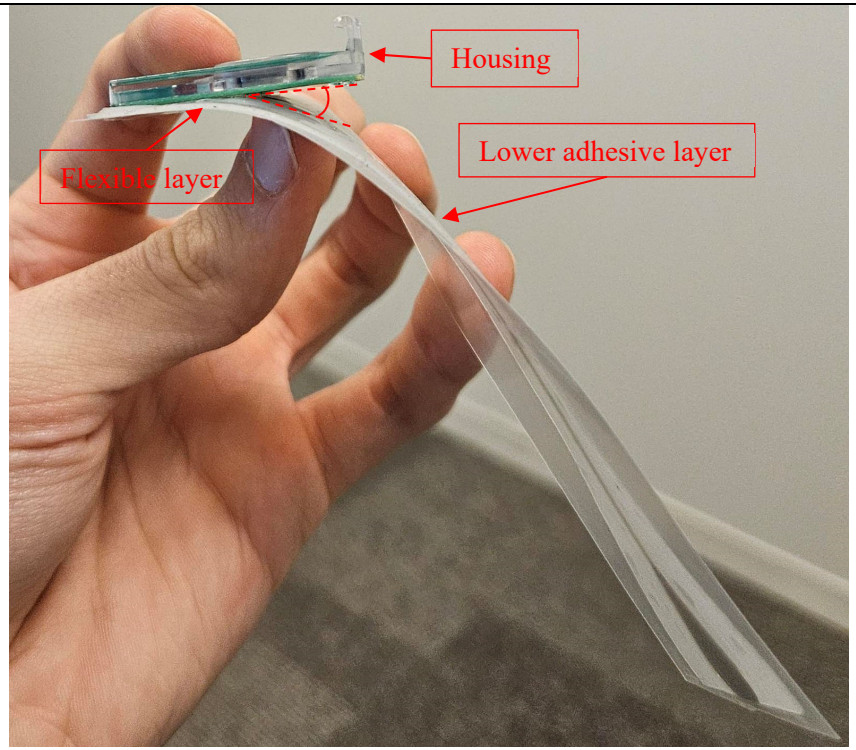

Infringement of U.S. Patent No. 12,274,554
By the Bardy CAM Patch Product

	Carnation Ambulatory Monitor™ 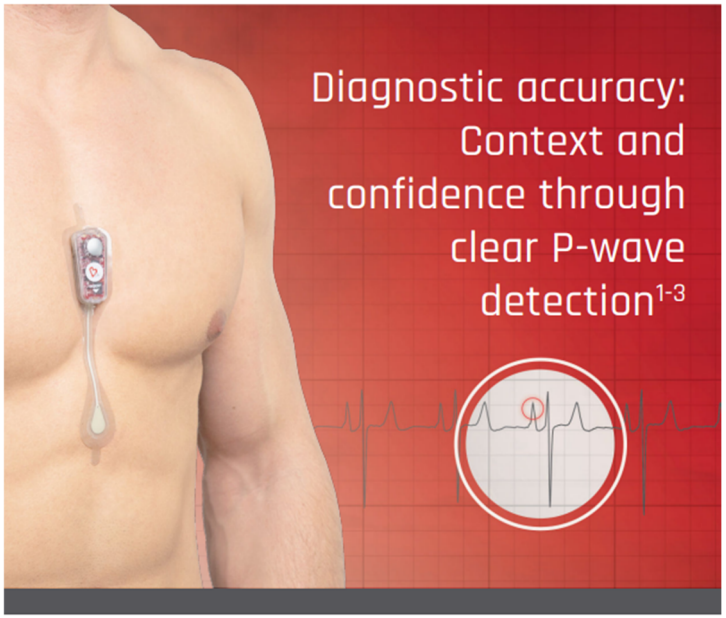 BardyDx® (https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM-Brochure.pdf)